



DME: CHARGEABLE SUPPLIES

HOSPITAL INFORMATION SYSTEM (HIS)

INTERPROFESSIONAL REHAB, ALLIED HEALTH & NURSING

Ordering DME: Chargeable Supplies

1. Physician will navigate to Quick Order Fracture M-Page.
2. Click on the supply that is to be ordered.
3. Click on the green shopping cart to get to the orders for signature page. Click sign.

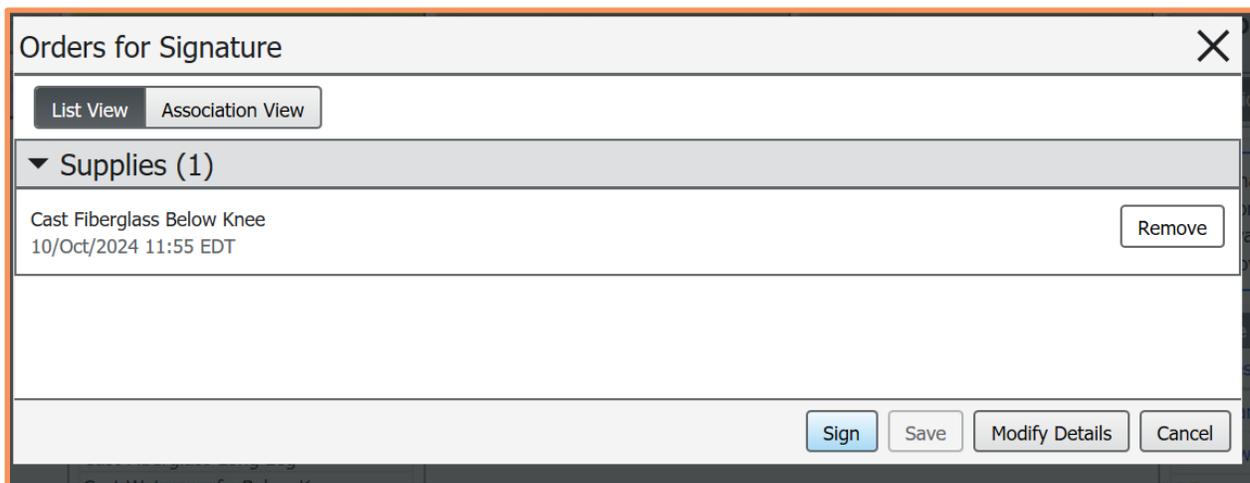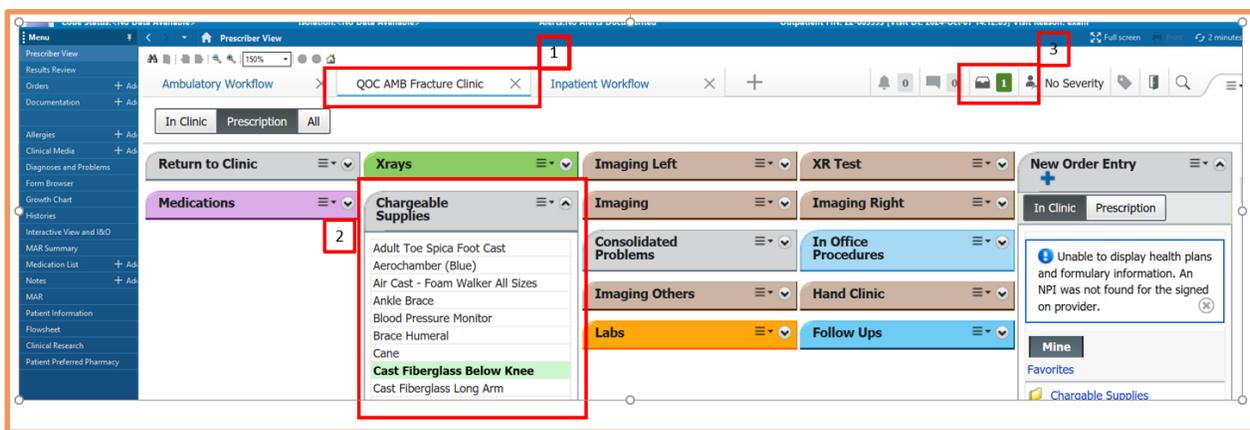

***Note:** Supplies orders can also be placed by searching for them in the Orders component from the Table of Contents (Blue bar).



DME: CHARGEABLE SUPPLIES

HOSPITAL INFORMATION SYSTEM (HIS)

Accessing and Documenting the PowerForm

4. The Clinician (ie: Ortho Tech, Therapists) will see the supply on the Activities and Interventions component on the Table of Contents.
 - ***Note:** Some end users will need to go to the Supplies tab when in Activities and Interventions or Multi Patient Task List.
5. Right Click in the gray box beside the supply Task.


MAR Summary		Thursday October 10, 2024 07:00:00 - Thursday October 10, 2024 19:00:00					
Interactive View and I&O		Office/Clinic Task					
Activities and Interventions		Task retrieval completed					
Orders	+ Add	Provider Name	Mnemonic	Task Status	Order Details	Order Status	Task Description
Documentation	+ Add	NHS Test01, Physician - Orthopaedic Surgery	Cast Fiberglass Below Knee	Pending	10/10/24 11:55:00 EDT	Ordered	Chargeable Supply

6. Click on “Chart Details...” and the PowerForm for AMB Supplies Dispensing will open up.

Office/Clinic Task		
Task retrieval completed		
	Provider Name	Mnemonic
	- Orthopaedic Surgery	Cast Fiberglass Below Knee
	- Vascular Surgery	diphenhydrAMINE
	- Vascular Surgery	dimenhydrINATE
	- Vascular Surgery	sodium chloride 0.9% intraven
	- Vascular Surgery	acetaminophen
	- Vascular Surgery	sodium chloride 0.9% intraven
	- Vascular Surgery	hydrocortisone (hydrocortison
	i, FRCPC	sodium chloride 0.9% intraven
	i, FRCPC	dimenhydrINATE
	i, FRCPC	diphenhydrAMINE
	i, FRCPC	acetaminophen
	i, FRCPC	diphenhydrAMINE
	i, FRCPC	ferric derisomaltose
	i, FRCPC	hydrocortisone (hydrocortison
	i, FRCPC	sodium chloride 0.9% intraven

***Note:** End user can also double click anywhere along the Task line to open the PowerForm.

- Complete the PowerForm and sign the power form with the green check mark (see PowerForm tip sheet for more information)

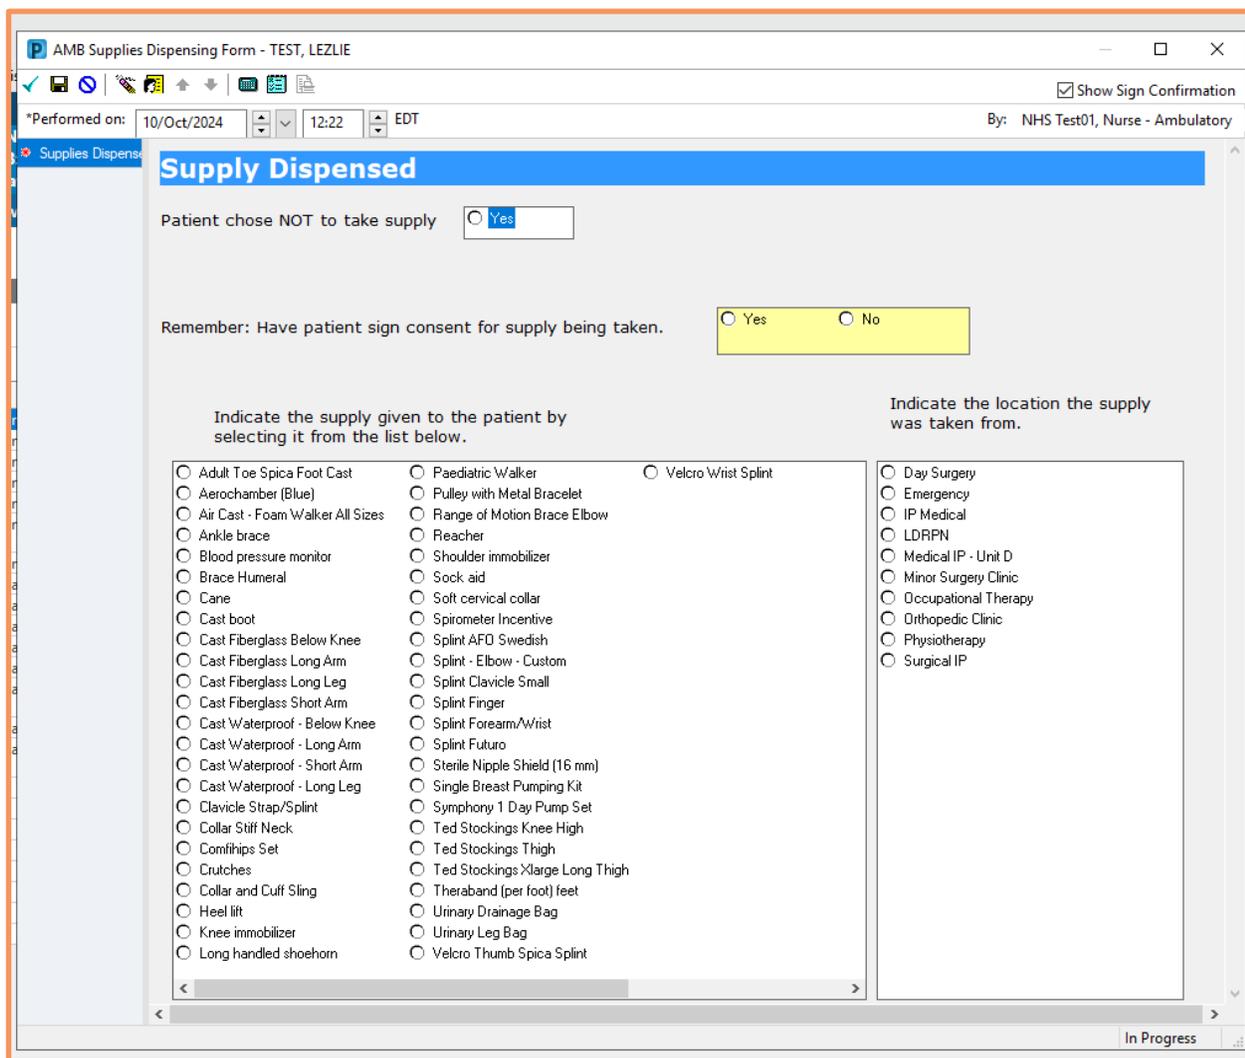

AMB Supplies Dispensing Form - TEST, LEZLIE

Show Sign Confirmation

*Performed on: 10/Oct/2024 12:22 EDT By: NHS Test01, Nurse - Ambulatory

Supply Dispersed

Patient chose NOT to take supply Yes

Remember: Have patient sign consent for supply being taken. Yes No

Indicate the supply given to the patient by selecting it from the list below.

Indicate the location the supply was taken from.

<input type="radio"/> Adult Toe Spica Foot Cast	<input type="radio"/> Paediatric Walker	<input type="radio"/> Velcro Wrist Splint	<input type="radio"/> Day Surgery
<input type="radio"/> Aerochamber (Blue)	<input type="radio"/> Pulley with Metal Bracelet		<input type="radio"/> Emergency
<input type="radio"/> Air Cast - Foam Walker All Sizes	<input type="radio"/> Range of Motion Brace Elbow		<input type="radio"/> IP Medical
<input type="radio"/> Ankle brace	<input type="radio"/> Reacher		<input type="radio"/> LDRPN
<input type="radio"/> Blood pressure monitor	<input type="radio"/> Shoulder immobilizer		<input type="radio"/> Medical IP - Unit D
<input type="radio"/> Brace Humeral	<input type="radio"/> Sock aid		<input type="radio"/> Minor Surgery Clinic
<input type="radio"/> Cane	<input type="radio"/> Soft cervical collar		<input type="radio"/> Occupational Therapy
<input type="radio"/> Cast boot	<input type="radio"/> Spirometer Incentive		<input type="radio"/> Orthopedic Clinic
<input type="radio"/> Cast Fiberglass Below Knee	<input type="radio"/> Splint AFO Swedish		<input type="radio"/> Physiotherapy
<input type="radio"/> Cast Fiberglass Long Arm	<input type="radio"/> Splint - Elbow - Custom		<input type="radio"/> Surgical IP
<input type="radio"/> Cast Fiberglass Long Leg	<input type="radio"/> Splint Clavicle Small		
<input type="radio"/> Cast Fiberglass Short Arm	<input type="radio"/> Splint Finger		
<input type="radio"/> Cast Waterproof - Below Knee	<input type="radio"/> Splint Forearm/Wrist		
<input type="radio"/> Cast Waterproof - Long Arm	<input type="radio"/> Splint Futuro		
<input type="radio"/> Cast Waterproof - Short Arm	<input type="radio"/> Sterile Nipple Shield (16 mm)		
<input type="radio"/> Cast Waterproof - Long Leg	<input type="radio"/> Single Breast Pumping Kit		
<input type="radio"/> Clavicle Strap/Splint	<input type="radio"/> Symphony 1 Day Pump Set		
<input type="radio"/> Collar Stiff Neck	<input type="radio"/> Ted Stockings Knee High		
<input type="radio"/> Comfithips Set	<input type="radio"/> Ted Stockings Thigh		
<input type="radio"/> Crutches	<input type="radio"/> Ted Stockings Xlarge Long Thigh		
<input type="radio"/> Collar and Cuff Sling	<input type="radio"/> Theraband (per foot) feet		
<input type="radio"/> Heel lift	<input type="radio"/> Urinary Drainage Bag		
<input type="radio"/> Knee immobilizer	<input type="radio"/> Urinary Leg Bag		
<input type="radio"/> Long handled shoehorn	<input type="radio"/> Velcro Thumb Spica Splint		

In Progress

Patient Consent Completion and Scanning

- Have the patient sign the patient consent form that they took the supply and consented to the charge (this process is not changing).
- The consent will be scanned into the patient chart by the person assigned to this responsibility. (see WQM tip sheet for scanning information).